



## 非イオン界面活性剤の分離

### Triton X-100


SunShell C18 2.6  $\mu$ m, 150 x 3.0 mm i.d.

Mobile phase: Tetrahydrofuran:Acetonitrile:Water = **0:50:50**


1. Triton X 100

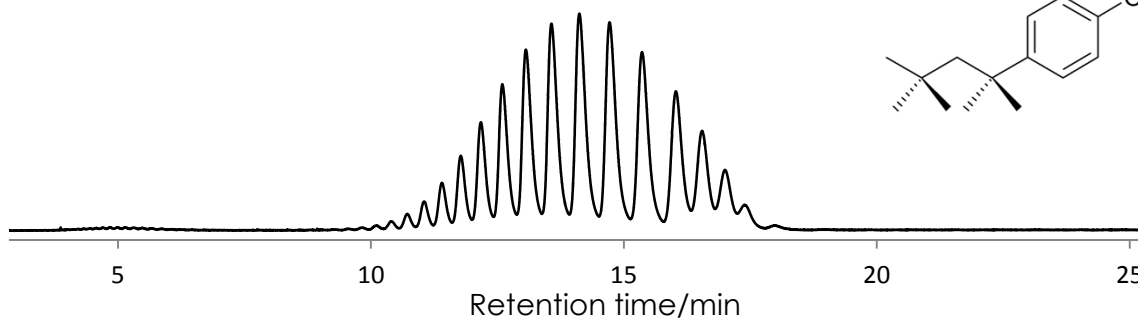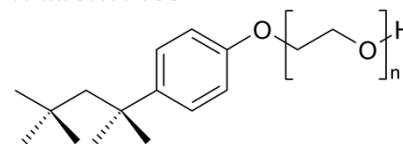

Mobile phase: Tetrahydrofuran:Acetonitrile:Water = **10:35:55**

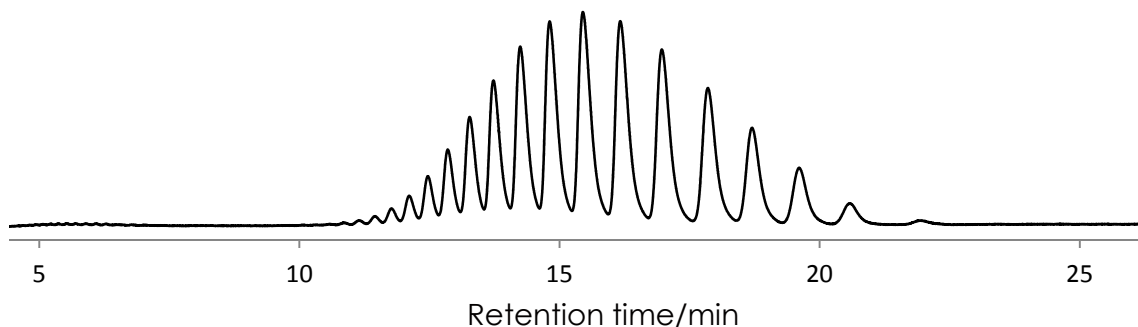

Mobile phase: Tetrahydrofuran:Acetonitrile:Water = **20:20:60**

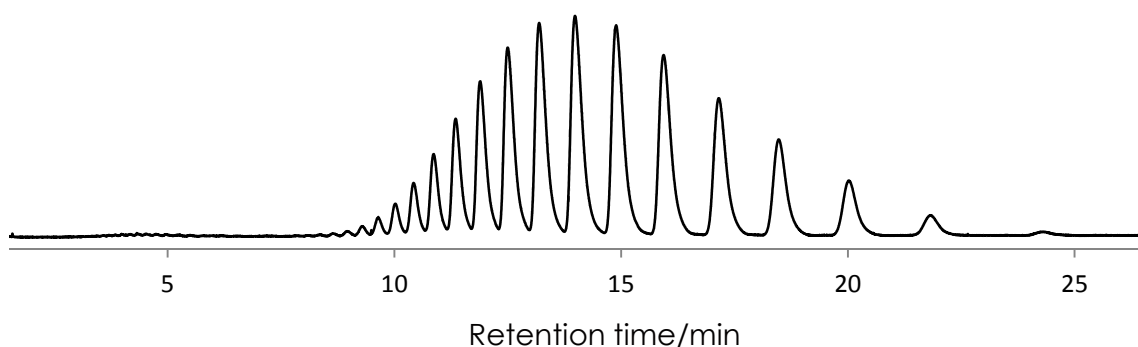

Column: SunShell C18, 2.6  $\mu$ m 150 x 3.0 mm i.d.

Mobile phase: Tetrahydrofuran:Acetonitrile:Water  
= 0:50:50, 10:35:55, 20:20:60

Flow rate: 0.5 mL/min

Temperature: 25  $^{\circ}$ C

Detection: UV@275nm

Sample: 1= Triton X-100

Instrument	Hitachi Chromaster®
Detector:	5410
Oven:	5310
AutoSampler:	5260
Pump:	5160

